

Henry Ford Health

Henry Ford Health Scholarly Commons

Women's Health Articles

Obstetrics, Gynecology and Women's Health
Services

1-1-2020

The impact of a wireless audio system on communication in robotic-assisted laparoscopic surgery: A prospective controlled trial.

Ziv Tsafirir
Henry Ford Health

Kirsten Janosek-Albright
Henry Ford Health

Joelle Aoun
Henry Ford Health

Mireya Diaz-Insua
Henry Ford Health, MInsua1@hfhs.org

Abd-El-Rahman Abd-El-Barr
Henry Ford Health

See next page for additional authors

Follow this and additional works at: https://scholarlycommons.henryford.com/womenshealth_articles

Recommended Citation

Tsafirir Z, Janosek-Albright K, Aoun J, Diaz-Insua M, Abd-El-Barr AE, Schiff L, Talukdar S, Menon M, Munkarah A, Theoharis E, and Eisenstein D. The impact of a wireless audio system on communication in robotic-assisted laparoscopic surgery: A prospective controlled trial. PLoS One 2020; 15(1):e0220214.

This Article is brought to you for free and open access by the Obstetrics, Gynecology and Women's Health Services at Henry Ford Health Scholarly Commons. It has been accepted for inclusion in Women's Health Articles by an authorized administrator of Henry Ford Health Scholarly Commons.

Authors

Ziv Tsafrir, Kirsten Janosek-Albright, Joelle Aoun, Mireya Diaz-Insua, Abd-El-Rahman Abd-El-Barr, Lauren Schiff, Shobhana Talukdar, Mani Menon, Adnan R. Munkarah, Evan Theoharis, and David Eisenstein


RESEARCH ARTICLE

The impact of a wireless audio system on communication in robotic-assisted laparoscopic surgery: A prospective controlled trial

Ziv Tsafirir^{1,2*}, Kirsten Janosek-Albright³, Joelle Aoun¹, Mireya Diaz-Insua³, Abd-El-Rahman Abd-El-Barr³, Lauren Schiff¹, Shobhana Talukdar¹, Mani Menon³, Adnan Munkarah¹, Evan Theoharis¹, David Eisenstein¹

1 Minimally Invasive Gynecologic Surgery, Women's Health Services, Henry Ford Hospital, Detroit, Michigan, **2** Department of Obstetrics and Gynecology, Kaplan medical Center, Rehovot, Affiliated to the Faculty of Medicine, the Hebrew University, Jerusalem, Israel, **3** Vattikuti Urology Institute, Henry Ford Hospital, Detroit, Michigan

* zivtsafirir@gmail.com, tazivtz@clalit.org.il



OPEN ACCESS

Citation: Tsafirir Z, Janosek-Albright K, Aoun J, Diaz-Insua M, Abd-El-Barr A-E-R, Schiff L, et al. (2020) The impact of a wireless audio system on communication in robotic-assisted laparoscopic surgery: A prospective controlled trial. PLoS ONE 15(1): e0220214. <https://doi.org/10.1371/journal.pone.0220214>

Editor: Isaac Yi Kim, The Cancer Institute of New Jersey, Robert Wood Johnson Medical School, UNITED STATES

Received: July 6, 2019

Accepted: November 25, 2019

Published: January 10, 2020

Copyright: © 2020 Tsafirir et al. This is an open access article distributed under the terms of the [Creative Commons Attribution License](https://creativecommons.org/licenses/by/4.0/), which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.

Data Availability Statement: All relevant data are within the manuscript and its Supporting Information files.

Funding: The wireless headsets were supplied by Quail Digital; Blue Cross Blue Shield Michigan Foundation supported this study; grant number 2174. PIRAP (\$10000 grant); and the Graduate Medical Education Research Committee of the Henry Ford Health System supported this study;

Abstract

Background

Robotic surgery presents a challenge to effective teamwork and communication in the operating theatre (OR). Our objective was to evaluate the effect of using a wireless audio headset device on communication, efficiency and patient outcome in robotic surgery.

Methods and findings

A prospective controlled trial of team members participating in gynecologic and urologic robotic procedures between January and March 2015. In the first phase, all surgeries were performed without headsets (control), followed by the intervention phase where all team members used the wireless headsets. Noise levels were measured during both phases. After each case, all team members evaluated the quality of communication, performance, teamwork and mental load using a validated 14-point questionnaire graded on a 1–10 scale. Higher overall scores indicated better communication and efficiency. Clinical and surgical data of all patients in the study were retrieved, analyzed and correlated with the survey results. The study included 137 procedures, yielding 843 questionnaires with an overall response rate of 89% (843/943). Self-reported communication quality was better in cases where headsets were used (113.0 ± 1.6 vs. 101.4 ± 1.6 ; $p < .001$). Use of headsets reduced the percentage of time with a noise level above 70 dB at the console ($8.2\% \pm 0.6$ vs. $5.3\% \pm 0.6$, $p < .001$), but had no significant effect on length of surgery nor postoperative complications.

Conclusions

The use of wireless headset devices improved quality of communication between team members and reduced the peak noise level in the robotic OR.

grant number 1407 (\$5000 grant). Drs. Tsafir, Janosek-Albright, Aoun, Diaz-Insua, Abd-El-Barr, Schiff, Talukdar, Menon, Munkarah, Theoharis and Eisenstein have no other conflicts of interest or financial ties to disclose except of what is disclosed above. The funders had no role in study design, data collection and analysis, decision to publish, or preparation of the manuscript.

Competing interests: The wireless headsets were supplied by Quail Digital; Blue Cross Blue Shield Michigan Foundation supported this study; grant number 2174. PIRAP (\$10000 grant); and the Graduate Medical Education Research Committee of the Henry Ford Health System supported this study; grant number 1407 (\$5000 grant). Drs. Tsafir, Janosek-Albright, Aoun, Diaz-Insua, Abd-El-Barr, Schiff, Talukdar, Menon, Munkarah, Theoharis and Eisenstein have no other conflicts of interest or financial ties to disclose except of what is disclosed above. The funders had no role in study design, data collection and analysis, decision to publish, or preparation of the manuscript. Specifically, Quail Digital had no role in study design, data collection and analysis, decision to publish, or preparation of the manuscript. This statement does not alter our adherence to PLOS ONE policies on sharing data and materials.

Introduction

There is strong evidence in the literature that supports the importance of effective communication and teamwork in regards to patient safety in the operating room (OR) [1, 2]. Event analysis has found that deficiencies in teamwork and communication contribute to adverse events, thus demonstrating that nontechnical skills are as important as technical surgical skills in preventing adverse patient outcomes [3, 4].

Communication is defined as “a process by which information is exchanged between individuals through a common system of symbols, signs, or behavior” [5]. Communication in the OR relies heavily on speech, but also encompasses visual and physical cues. Due to the large footprint platform of the robot, team members are physically separated in space, and thus face-to-face interaction during the surgery is severely limited. Unlike the conventional OR setting, robotic surgeons must rely primarily on auditory means of communication, unaided by visual cues [6–8]. In addition, studies have shown that increased noise during surgery was associated with a greater risk for postoperative complications [9, 10]. The robotic platform possibly lead to increased noise in the OR, which could present a source for errors and impaired safety and efficiency during surgery. As the adoption of robotic surgery is expanding at a rapid rate, these concerns become relevant and may present an unforeseen source of complications.

Our team sought a novel technological solution that has been used in other settings to improve auditory communication. The primary objective of our study was to determine whether a wireless audio headset improves the quality of communication in robotic surgery. Secondary objectives were to assess the impact of using such device on the noise level during robotic procedures, efficiency and patient outcomes.

Materials and methods

This study design was a non-randomized, prospective controlled trial.

The study was approved by the Henry Ford Health System IRB, approval number 8984. All participants gave written informed consent before the start of the study.

Patients included in the study had surgery performed by the Departments of Gynecology and Urology in the Henry Ford Health System, a large vertically integrated health system in southeast Michigan. The most common robotic procedures performed by each department were included in the study, which were the following: total hysterectomy, prostatectomy and nephrectomy.

Study participants belonged to the following OR team categories: surgeons, surgeons' assistants (including fellows, residents and certified first assistants), surgical technicians, circulating nurses, and anesthesiologists or certified registered nurse anesthetists. Prior to study initiation, every participant signed an informed consent and was subsequently assigned a study identifier to maintain participant anonymity. In addition, participants filled out a demographic questionnaire that included information regarding their age, gender, role in the robotic OR and their years of experience in that role.

At the end of each surgery, all team members evaluated the quality of communication, performance, teamwork, and mental load using a 14-item questionnaire based on previously published validated questionnaire [11, 12]. Agreement with the statement presented in each item was graded on a 10-point Likert scale (S1 Table).

In the first phase of the study, the control period, team members did not use the headset device during surgery. Following accrual of adequate cases (see power calculations) for baseline data, the same participants proceeded to the second phase of the study, the intervention



Fig 1. Quail digital wireless headset.

<https://doi.org/10.1371/journal.pone.0220214.g001>

period, which involved the use of the headset device by all team members during the procedure. Through both phases of the study, participants filled out the questionnaire.

The Quail Digital Healthcare headset system that was used is a digital audio hands free, wireless headset device with noise cancellation capabilities that weighs 23 gm (Quail Digital, London, UK) (Fig 1), covering one ear only.

In addition, decibel-recording devices (TES-1352H, Taipei, Taiwan) were used during each case to monitor the noise level in the OR in both phases of the study. In each OR, 2 such devices were installed: 1 at the bedside (B), and 1 at the surgeon's console (C). Ambient OR noise (dB) were continuously recorded and stored in 1-second intervals. Furthermore, background noise readings were taken once from each OR at the end of the trial. The background noise levels were subtracted from OR recordings.

The following patient clinical data were retrospectively retrieved from the electronic medical records: demographics, past medical and surgical history, body mass index, indication for surgery, type of surgery, time to complete the surgery, perioperative and postoperative complications, length of stay and pathology findings. The Charlson scoring system was used to summarize the comorbidity of patients in both the control and study phases [13]. The severity of operative complications was graded according to the Clavien-Dindo classification [14]. Patient outcome data were correlated with the survey and noise data obtained from study participants.

Statistics

Questionnaire scoring. To summarize the questionnaire, an overall score was calculated. Scores from statements presented in a negative tone, e.g. "I had to repeat myself because people didn't understand/hear my message the first time," were subtracted from 10, so that all items could contribute in the same direction towards the overall score; i.e. higher overall scores indicated better communication and efficiency.

Processing of noise data. An average background noise level per room was calculated from each microphone in 6 different operating rooms. This average was subtracted from each noise time series from the surgical cases matched to the corresponding microphone and OR. The average noise and the percentage of time that noise surpassed 70 dB during console

operation were calculated for each microphone in each case. These 2 measures were compared between the control and intervention groups using a linear regression model to account for the potential influence of the OR and team size.

Comparison of variables. Descriptive statistics were calculated and compared between groups. For patient characteristics the t-test and chi-square or Fisher exact tests were used to compare continuous and categorical variables respectively. The effect of headset use on patient outcomes was compared using a linear regression model that accounted for relevant patient characteristics and robotic experience of the surgical team (see below). The latter was calculated as the average experience in number of surgeries performed robotically among the team members for a given surgery. We had the number of surgeries classified in 6 groups (group 1 = 0–20 surgeries; group 2 = 21–40 surgeries; group 3 = 41–60 surgeries; group 4 = 61–80 surgeries; group 5 = 81–100; group 6 = more than 100 surgeries), and thus the average corresponds to the average class. This average class was included as a categorical variable in the model.

A linear mixed model was used for comparisons of individual item scores and overall score from the questionnaires between the groups to account for the clustered nature of the data. Significance was set at 0.05 for all comparisons.

Sample size calculation. Sample size for this trial was estimated considering operative time as the main outcome. A minimum of 50 procedures per arm were deemed necessary in order to detect a standardized difference of 0.50 in operative time between the 2 groups using a two-sided test at 80% power and significance level of 0.05. Based on historical schedules, such a size could be achieved by a 1-month period for each phase of the study.

Results

A total of 137 robotic procedures performed from January through March 2015 were included in the analysis. The study group (with headsets) contained 69 cases and the control (without headsets) contained 68 cases.

Baseline characteristics and procedure details are presented in [Table 1](#). No significant differences were found between the patients in the study and control groups in terms of body mass index, prior comorbidities, past surgical history, type of robotic surgery performed, use of the fourth robotic arm, and number of team members participating in the procedure.

A total of 148 team members participated in the study. Demographic data and work experience of all participants, stratified by role, are summarized in [Table 2](#). Overall 843 questionnaires were filled out, with a response rate of 89%. There was no significant difference in the response rate between the different team member categories ([Fig 2](#)).

Participants reported better overall communication in cases where headsets were used (113.0 ± 1.6 vs. 101.4 ± 1.6 ; $p < .001$) as measured by mean survey score. The mean score for individual items in both the study and control groups are shown in [Table 3](#). When stratified by responder's role, the overall scores were significantly higher while using the headsets, in comparison to the control. The mean score for each item with and without the headsets stratified by responder role is presented in [S2 Table](#).

Use of the headset did not reduce the noise level in the robotic OR, as there was no significant difference in average noise levels between the groups ([Table 4](#)). However, cases in which headsets were used demonstrated a lower percentage of time with noise level above 70 dB at the console ($8.2\% \pm 0.6$ vs. $5.3\% \pm 0.6$, $p < .001$) ([Table 4](#)). There were no differences between the study and control groups in regards to time to complete the surgery, estimated blood loss, length of hospital stay, or postoperative complications ([Table 4](#)). Similarly, there were no differences in outcomes after controlling for procedures type.

Table 1. Descriptive statistics of patients and procedures.

Variable	With headsets	Without headsets	p-value
	Mean ± SD(n = 69)	Mean ± SD(n = 68)	
Age (years)	58.6 ± 11.0	58.1 ± 12.1	.827
Body mass index (lb/inch ²)	30.4 ± 5.7	30.7 ± 6.4	.775
Variable	Counts (%)	Counts (%)	p-value
Sex: Males	42(61%)	41(60%)	1.000
Department: Gynecology	22(32%)	20(29%)	.853
Charlson score			.892
0	35(51%)	40(59%)	
1	20(29%)	10(15%)	
2	14(20%)	18(26%)	
Previous laparotomy			.674
Single	11(17%)	15(22%)	
Multiples	4(6%)	5(7%)	
Previous laparoscopy	12(19%)	13(19%)	1.000
Procedure			.504
Prostatectomy	31(45%)	31(46%)	
Hysterectomy	21(30%)	16(24%)	
Partial nephrectomy	6(9%)	11(16%)	
Radical nephrectomy	8(12%)	5(7%)	
Other ^a	3(4%)	5(7%)	
LND performed	25(45%)	26(50%)	.701
Use of a fourth robotic arm	41(59%)	35(51%)	.392
Frozen sections	31(45%)	27(40%)	.605
Surgical team size			.654
5 members	5(7%)	4(6%)	
6 members	18(26%)	11(16%)	
7 members	14(20%)	17(25%)	
8 members	14(20%)	20(29%)	
9 members	14(20%)	12(18%)	
10 members	4(6%)	4(6%)	

SD, standard deviation; LND, lymph node dissection

^aOther: Study group—Gynecology: 1 myomectomy, Urology—2 simple prostatectomies; Control group—Gynecology: 1 sub-total hysterectomy and 2 myomectomies, Urology—2 radical nephroureterectomy.

<https://doi.org/10.1371/journal.pone.0220214.t001>

Discussion

This study is the first to evaluate the impact of using wireless headsets on the quality of communication between different team members during robotic surgery. Our data shows that the use of such a device significantly improves the quality of communication in robotic surgery. However, these improvements did not reduce operation duration nor clinical outcomes for patients.

The last decade is characterized by a rapid adoption and dissemination of robotic technology and robotic-assisted minimally invasive surgery. In urology, for example, robotic-assisted radical prostatectomy was rapidly adopted to become the main surgical approach for treatment of localized prostate cancer, with an increasing rate from 8% in 2004 to 67% in 2010 [15]. Between 2005 and 2010, the rate of robotic hysterectomy increased from as low as 0.5% to as high as 22% [16]. It is estimated that approximately one-half of all minimally invasive

Table 2. Participants demographics^a.

Characteristic	Attending	Anesthesia ^b	Circulator	ST	Fellow	Resident	FA
N	13	54	21	11	5	20	4
Age (years)	49.7±7.3	41.1±11.4	45.8±11.2	43.0±12.9	38.0±5.3	30.9±2.4	40.0±4.1
Sex							
Females	2(15.4)	35(64.8)	19(90.5)	10(90.9)	1(20)	11(55.0)	4(100)
Males	11(84.6)	19(35.2)	2(9.5)	1(9.1)	4(80.0)	9(45.0)	0(0.0)
Experience (years)	16.9±9.5	9.8±10.3	15.6±12.8	9.2±12.8	5.0±5.4	3.1±1.5	10.0±10.8
Robotic experience							
0-20cases	1(7.7)	9(16.7)	5(23.8)	2(18.2)	0(0.0)	11(55.0)	0(0.0)
20-40cases	0(0.0)	5(9.3)	3(14.3)	2(18.2)	0(0.0)	5(25.0)	0(0.0)
40-60cases	2(15.4)	6(11.1)	2(9.5)	0(0.0)	0(0.0)	0(0.0)	0(0.0)
60-80cases	0(0.0)	7(13.0)	2(9.5)	2(18.2)	1(20.0)	0(0.0)	1(25.0)
80-100cases	0(0.0)	7(13.0)	1(4.8)	2(18.2)	0(0.0)	0(0.0)	0(0.0)
> 100 cases	10(76.9)	20(37.0)	8(38.1)	3(27.3)	4(80.0)	4(20.0)	3(75.0)

FA, first assistant; ST, surgical technician

^a128 of 148 participants provided the demographic information.

^bAnesthesia: Anesthesiologist/CRNA (certified registered nurse anesthetists)

Numbers represent mean ± standard deviation except for sex and robotic experience, which represent counts (%). Age and sex are distributed significantly different at $p < .001$, experience $p = .001$ and robotic experience $p = .013$.

<https://doi.org/10.1371/journal.pone.0220214.t002>

hysterectomies are now performed robotically [17, 18]. The rapid assimilation of the robotic platform is attributed to its hypothetical benefits, such as improved ergonomics, wider range of motion, 3-dimensional stereoscopic vision and enhanced visual magnification. However, adoption of such technology raised concerns about patient safety and surgical outcomes [19–21].

The causal relationship between communication failure in the OR and adverse patient outcomes is well established in the literature [1–3]. The Joint Commission identified breakdowns in communication as a leading root cause of operative or postoperative complication events [3]. In their observational study, Wiegmann and colleagues found that surgical errors increased significantly with increased disruptions and that teamwork and communication problems were the strongest predictors of surgical errors [22].

Only four studies have looked at the inherent communication challenges faced by team members in robotic surgery. Robotic surgery was associated with a higher volume of information exchanged within the OR team, compared with regular laparoscopy during cholecystectomy [8]. Specifically, there was a significant shift of communication in robotic OR towards verbal cues [6, 7].

Our prospective controlled trial is the first intervention aiming to improve communication and teamwork in the robotic OR. We focused on the most important part of communication in the robotic setting, which is verbal communication. With the assistance of the wireless headsets, we amplified the verbal cues. This intervention showed marked improvement in all 4 of the domains that were evaluated in the questionnaire: quality of communication, performance, teamwork, and mental load. Moreover, all team members, regardless of their role, shared the same positive perception of the added value of using the headsets in robotic cases.

Previous studies have found a correlation between the level of noise in the OR and postoperative complications [9, 10]. Kurman et al. measured the sound level during 35 elective open abdominal procedures and found that increased intraoperative noise volume was associated with surgical site infection [9]. In their prospective controlled trial, Engelmann and colleagues

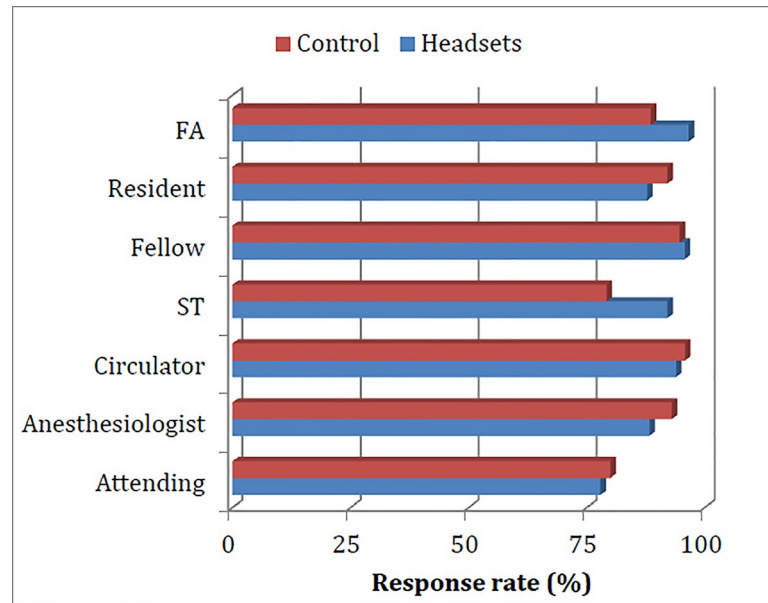


Fig 2. Response rate of team members, stratified by role. Abbreviations: FA, first assistant; ST, surgical technician.

<https://doi.org/10.1371/journal.pone.0220214.g002>

assessed the impact of a noise reduction program in a pediatric OR. Sound levels were measured and surgical complications recorded before and after implementation of a noise reduction protocol. The intervention significantly reduced the noise level in the OR. Additionally, the incidence of postoperative complications was significantly lower among the patients in the intervention group [10].

Our data showed that in cases where headsets were used there was a decreased period of time with noise level above 70 dB at the robotic console. This level of noise is equivalent to a domestic vacuum cleaner [23]. However, there was no significant difference in the average noise level between both groups. Together, these data suggest that reduction in peak noise duration is not sufficient to improve patient outcomes and a reduction in the average noise levels is necessary.

Although noise was significantly reduced only at peak levels, our data demonstrated that team members perceived communication to be better while using the headsets. Specifically, participants commented that they could hear clearly during the case, needed to repeat themselves less and were less bothered or distracted by the noise in the OR when using the device. This can be attributed to the noise cancelling capabilities of the headsets, which simultaneously reduces ambient noise and increases voice clarity for the user.

Our study has its own limitations. Firstly, this study was not randomized because the team members themselves were the study participants, and randomization was not feasible due to a lack of consistency of participants assigned to cases during the study period. Additionally, the decision to start with the control phase first was based on the concern that team members could potentially be biased by the prior use of the headset device.

Despite the use of validated questionnaires, our results may have been subject to responder bias. Participants who had a good experience with the headsets might be more enthusiastic to fill out the survey at the end of the case, as compared to participants who did not have a good experience with the headsets. This could potentially skew results in favor of this device. However, the fact that we had a response rate of 89% with no significant difference in the response

Table 3. Mean scores for individual items of the survey^a.

Variable	With headsets Mean ± SE	Without headsets Mean ± SE	p-value
Heard clearly during case	9.0±0.2	7.2±0.2	< .001
Needed to repeat	7.6±0.2	5.9±0.2	< .001
Team communication	8.6±0.1	7.5±0.1	< .001
Focus	8.5±0.1	8.0±0.1	< .001
Steps took longer	7.8±0.2	6.3±0.2	< .001
Feel safe	8.9±0.1	8.3±0.1	< .001
Successful in task	8.8±0.1	8.5±0.1	< .001
High team morale	8.9±0.1	8.4±0.1	< .001
Participation	8.9±0.1	8.6±0.1	< .001
Efficient teamwork	9.0±0.1	8.4±0.1	< .001
Felt exhausted	7.0±0.2	6.3±0.2	< .001
Felt stressed/irritated	7.5±0.2	7.0±0.2	< .001
Hard work for task	5.8±0.2	5.3±0.2	< .001
Noise bothered/distracted	7.5±0.2	6.8 ± 0.2	< .001

SE, standard error

^aFor the full version of each statement please refer to [S1 Table](#).

<https://doi.org/10.1371/journal.pone.0220214.t003>

rates by participant’s role suggests that such potential bias was negligible. Finally, only ambient noise levels were measured in the OR. We recognize that measuring the decibel level inside the headsets would better reflect the actual noise reduction each team member experienced. However, given that the headset covers only one ear, team members were still exposed to and influenced by the ambient noise at the OR.

Table 4. Outcomes comparison by use of headsets.

Variable	With headsets Mean ± SE	Without headsets Mean ± SE	p-value
Overall score ^a	113.0±1.6	101.4±1.6	< .001
Noise level—average C (dB) ^b	64.1±0.4	64.8±0.4	.093
Noise level—average B (dB) ^b	66.2±0.5	66.3±0.4	.767
Noise level—above 70dB C (%) ^b	5.3±0.6	8.2±0.6	< .001
Noise level—above 70dB B (%) ^b	14.0±2.1	15.2±2.1	.595
Estimated blood loss (ml) ^c	117.1±34.3	112.3±31.2	0.883
Total time (min) ^c	296.0±16.6	277.2±15.1	0.240
Cut-close time (min) ^c	228.0±15.2	205.2±13.8	0.119
Console time (min) ^c	152.1±10.3	156.0±9.5	0.692
Postoperative complications Clavien-Dindo [14] Grades II-V (n)	5	6	.975
Length of stay (days) ^c	2.2±0.2	2.0±0.2	0.433

B, bedside; C, console; SE, standard error

^aAdjusted by operating room and role of the responder within the surgical team.

^bBackground-corrected noise adjusted by operating room and team size.

^cAdjusted by patient’s age, sex, body mass index, diagnosis, average robotic experience of the team and procedure type.

<https://doi.org/10.1371/journal.pone.0220214.t004>

Conclusion

We present here a novel approach to address a communication challenge in robotic procedures. Our study shows that the use of wireless headsets improves communication in the robotic OR. In addition, the percentage of time above a peak sound level of 70 dB is reduced while using headsets. These changes did not affect the clinical outcomes.

Supporting information

S1 Table. Questionnaire.

(DOCX)

S2 Table. The mean score for each statement with and without the headsets, stratified by responder role.

(DOCX)

Acknowledgments

We thank Dr. Amir Shafat, National University of Ireland Galway, for scientific discussion and editorial assistance. We thank Ms. Stephanie Stebens for editorial assistance.

Author Contributions

Conceptualization: Ziv Tsafrir, Kirsten Janosek-Albright, Joelle Aoun, Mireya Diaz-Insua, Lauren Schiff, Shobhana Talukdar, Mani Menon, Adnan Munkarah, Evan Theoharis, David Eisenstein.

Data curation: Ziv Tsafrir, Kirsten Janosek-Albright, Joelle Aoun, Mireya Diaz-Insua, Abd-El-Rahman Abd-El-Barr, Lauren Schiff, Shobhana Talukdar, Mani Menon, Adnan Munkarah, Evan Theoharis, David Eisenstein.

Formal analysis: Mireya Diaz-Insua, David Eisenstein.

Investigation: Ziv Tsafrir, Kirsten Janosek-Albright, Joelle Aoun, Abd-El-Rahman Abd-El-Barr, Lauren Schiff, Shobhana Talukdar, Mani Menon, Adnan Munkarah, Evan Theoharis, David Eisenstein.

Methodology: Ziv Tsafrir, Kirsten Janosek-Albright, Joelle Aoun, Mireya Diaz-Insua, Abd-El-Rahman Abd-El-Barr, Lauren Schiff, Mani Menon, Adnan Munkarah, Evan Theoharis, David Eisenstein.

Project administration: Ziv Tsafrir, Kirsten Janosek-Albright, Abd-El-Rahman Abd-El-Barr, Lauren Schiff, Mani Menon, Adnan Munkarah, Evan Theoharis, David Eisenstein.

Resources: Ziv Tsafrir, Kirsten Janosek-Albright, Joelle Aoun, Lauren Schiff.

Software: Mireya Diaz-Insua.

Supervision: Ziv Tsafrir, Kirsten Janosek-Albright, Joelle Aoun, Mireya Diaz-Insua, Abd-El-Rahman Abd-El-Barr, Shobhana Talukdar, Mani Menon, Adnan Munkarah, Evan Theoharis, David Eisenstein.

Validation: Mireya Diaz-Insua, David Eisenstein.

Visualization: Kirsten Janosek-Albright, Joelle Aoun, Abd-El-Rahman Abd-El-Barr, Shobhana Talukdar.

Writing – original draft: Ziv Tsafrir, Kirsten Janosek-Albright, Joelle Aoun, Mireya Diaz-Insua, Abd-El-Rahman Abd-El-Barr, Lauren Schiff, Shobhana Talukdar, Mani Menon, Adnan Munkarah, Evan Theoharis, David Eisenstein.

Writing – review & editing: Ziv Tsafrir, Joelle Aoun, Mireya Diaz-Insua, David Eisenstein.

References

1. Gawande AA, Zinner MJ, Studdert DM, Brennan TA. Analysis of errors reported by surgeons at three teaching hospitals. *Surgery*. 2003; 133:614–21. <https://doi.org/10.1067/msy.2003.169> PMID: 12796727
2. Lingard L, Espin S, Whyte S, Regehr G, Baker G, Reznick R, et al. Communication failures in the operating room: an observational classification of recurrent types and effects. *Qual Saf Health Care*. 2004; 13:330–4. <https://doi.org/10.1136/qshc.2003.008425> PMID: 15465935
3. Joint Commission. Sentinel event data: root causes by event type 2004–2Q 2015. Available at: http://www.jointcommission.org/assets/1/18/Root_Causes_Event_Type_2004-2Q_2015.pdf. Accessed August 26, 2015.
4. Hull L, Arora S, Aggarwal R, Darzi A, Vincent C, Sevdalis N. The impact of nontechnical skills on technical performance in surgery: a systematic review. *J Am Coll Surg*. 2012; 214:214–30. <https://doi.org/10.1016/j.jamcollsurg.2011.10.016> PMID: 22200377
5. Communication. *Merriam-Webster Collegiate Dictionary*. 11th ed. Springfield, MA: Meriam-Webster, Inc; 2003: 251.
6. Webster JL, Cao CG. Lowering communication barriers in operating room technology. *Hum Factors*. 2006; 48:747–58. <https://doi.org/10.1518/001872006779166271> PMID: 17240722
7. Nyssen A-S, Balvier A. Verbal communication as a sign of adaptation in socio-technical systems: the case of robotic surgery. Proceedings of the NDM9, 9th International Conference on Naturalistic Decision Making. London: British Computer Society; 2009:267–72.
8. Cao CGL, Taylor H. Effects of new technology on the operating room team. In: Khalid HM, Helander MG, Yeo AW, eds. *Work with Computing Systems*. Kuala Lumpur: Damai Sciences; 2004:309–12.
9. Kurmann A, Peter M, Tschan F, Muhlemann K, Candinas D, Beldi G. Adverse effect of noise in the operating theatre on surgical-site infection. *Br J Surg*. 2011; 98:1021–5. <https://doi.org/10.1002/bjs.7496> PMID: 21618484
10. Engelmann CR, Neis JP, Kirschbaum C, Grote G, Ure BM. A noise-reduction program in a pediatric operation theatre is associated with surgeon's benefits and a reduced rate of complications: a prospective controlled clinical trial. *Ann Surg*. 2014; 259:1025–33. <https://doi.org/10.1097/SLA.000000000000253> PMID: 24394594
11. Sexton JB, Helmreich RL, Neilands TB, Rowan K, Vella K, Boydan J, et al. The Safety Attitudes Questionnaire: psychometric properties, benchmarking data, and emerging research. *BMC Health Serv Res*. 2006; 6:44. <https://doi.org/10.1186/1472-6963-6-44> PMID: 16584553
12. Watts BV, Percarpio K, West P, Mills PD. Use of the Safety Attitudes Questionnaire as a measure in patient safety improvement. *J Patient Saf*. 2010; 6:206–9. <https://doi.org/10.1097/pts.0b013e3181fbbe86> PMID: 21500606
13. Charlson ME, Pompei P, Ales KL, MacKenzie CR. A new method of classifying prognostic comorbidity in longitudinal studies: development and validation. *J Chronic Dis*. 1987; 40:373–83. [https://doi.org/10.1016/0021-9681\(87\)90171-8](https://doi.org/10.1016/0021-9681(87)90171-8) PMID: 3558716
14. Dindo D, Demartines N, Clavien PA. Classification of surgical complications: a new proposal with evaluation in a cohort of 6336 patients and results of a survey. *Ann Surg*. 2004; 240:205–13. <https://doi.org/10.1097/01.sla.0000133083.54934.ae> PMID: 15273542
15. Lowrance WT, Eastham JA, Savage C, Maschino AC, Laudone VP, Christopher B, et al. Contemporary open and robotic radical prostatectomy practice patterns among urologists in the United States. *J Urol*. 2012; 187:2087–92. <https://doi.org/10.1016/j.juro.2012.01.061> PMID: 22498227
16. Smorgick N, As-Sanie S. The benefits and challenges of robotic-assisted hysterectomy. *Curr Opin Obstet Gynecol*. 2014; 26:290–4. <https://doi.org/10.1097/GCO.0000000000000080> PMID: 24914631
17. Anderson JE, Chang DC, Parsons JK, Talamini MA. The first national examination of outcomes and trends in robotic surgery in the United States. *J Am Coll Surg*. 2012; 215:107–14. <https://doi.org/10.1016/j.jamcollsurg.2012.02.005> PMID: 22560318
18. Tsui C, Klein R, Garabrant M. Minimally invasive surgery: national trends in adoption and future directions for hospital strategy. *Surg Endosc*. 2013; 27:2253–7. <https://doi.org/10.1007/s00464-013-2973-9> PMID: 23660720

19. Lee YL, Kilic GS, Phelps JY. Medicolegal review of liability risks for gynecologists stemming from lack of training in robot-assisted surgery. *J Minim Invasive Gynecol*. 2011; 18:512–5. <https://doi.org/10.1016/j.jmig.2011.04.002> PMID: 21777841
20. Lenihan JP Jr. Navigating credentialing, privileging, and learning curves in robotics with an evidence and experience-based approach. *Clin Obstet Gynecol*. 2011; 54:382–90. <https://doi.org/10.1097/GRF.0b013e31822b47e2> PMID: 21857169
21. Murphy DG, Bjartell A, Ficarra V, Graefen M, Haese A, Montironi R, et al. Downsides of robot-assisted laparoscopic radical prostatectomy: limitations and complications. *Eur Urol*. 2010; 57:735–46. <https://doi.org/10.1016/j.eururo.2009.12.021> PMID: 20036784
22. Wiegmann DA, ElBardissi AW, Dearani JA, Daly RC, Sundt TM 3rd. Disruptions in surgical flow and their relationship to surgical errors: an exploratory investigation. *Surgery*. 2007; 142:658–65. <https://doi.org/10.1016/j.surg.2007.07.034> PMID: 17981185
23. Sengpiel E. Decibel table, SPL, loudness comparison chart. Available at: www.sengpielaudio.com/TableOfSoundPressureLevels.htm. Accessed August 26, 2015.